

## Dental Materials Journal

53

H Index

**Country** Japan -  SCIMAGO INSTITUTIONS RANKINGS

**Subject Area and Category** Dentistry  
Dentistry (miscellaneous)

Materials Science  
Ceramics and Composites

**Publisher** Japanese Society for Dental Materials and Devices


**Publication type** Journals

**ISSN** 18811361, 02874547


**Coverage** 1982-2020

**Scope** Dental Materials Journal is a peer review journal published by the Japanese Society for Dental Materials and Devises aiming to introduce the progress of the basic and applied sciences in dental materials and biomaterials. The dental materials-related clinical science and instrumental technologies are also within the scope of this journal. The materials dealt include synthetic polymers, ceramics, metals and tissue-derived biomaterials. Forefront dental materials and biomaterials used in developing filed, such as tissue engineering, bioengineering and artificial intelligence, are positively considered for the review as well. Recent acceptance rate of the submitted manuscript in the journal is around 30%.


Quartiles

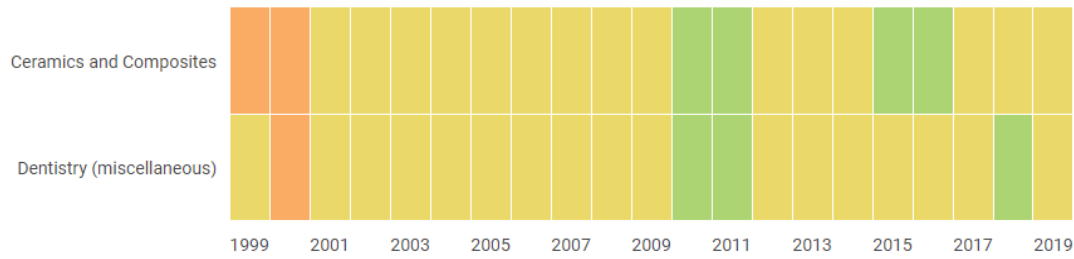


SJR

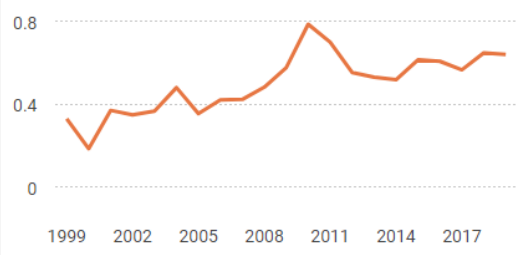


Citations per document

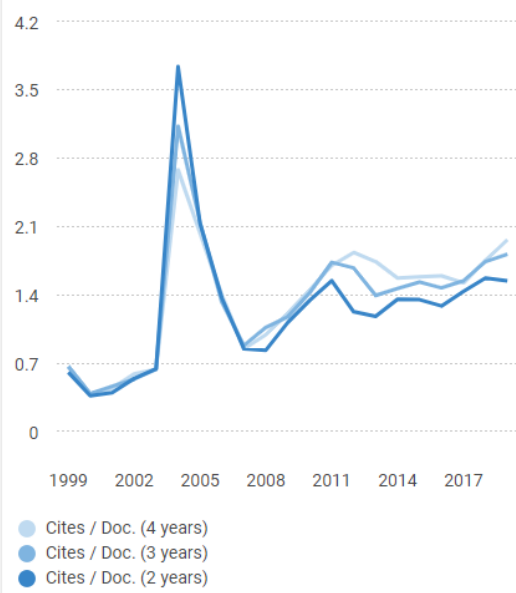


Total Cites Self-Cites

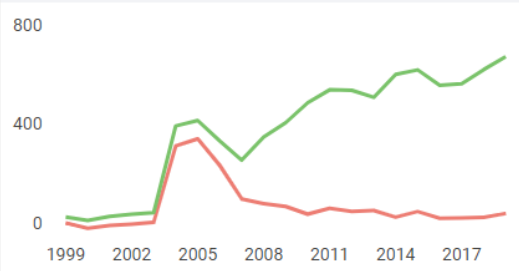

Citable documents Non-citable documents

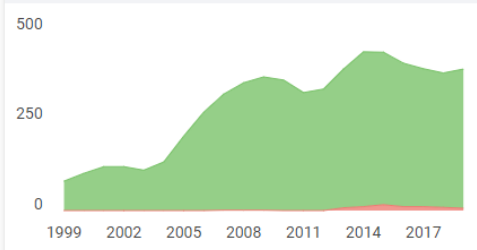

Cited documents Uncited documents

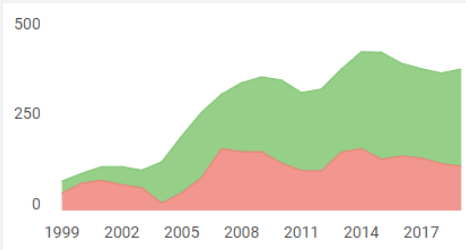

Dental Materials Journal

Q2

Ceramics and Composites

best quartile

SJR 2019  
0.64

powered by scimagojr.com

Show this widget in your own website

Just copy the code below and paste within your html code:

```
<a href="https://www.scima
```

Journal Profile																																										
Journal Title	DENTAL MATERIALS JOURNAL																																									
Journal Title Abbreviations	DENT MATER J																																									
ISSN	0287-4547																																									
E-ISSN	1881-1361																																									
h-index	50																																									
CiteScore	<table border="1"> <thead> <tr> <th>CiteScore</th> <th>SJR</th> <th>SNIP</th> <th colspan="3">CiteScore Rank</th> </tr> </thead> <tbody> <tr> <td>2.60</td> <td>0.642</td> <td>0.979</td> <td>Subject field</td> <td>Quartiles</td> <td>Rank</td> <td>Percentile</td> </tr> <tr> <td></td> <td></td> <td></td> <td>Category: Materials Science</td> <td>Q2</td> <td>49 / 106</td> <td>54%</td> </tr> <tr> <td></td> <td></td> <td></td> <td>Subcategory: Ceramics and Composites</td> <td></td> <td></td> <td></td> </tr> <tr> <td></td> <td></td> <td></td> <td>Category: Materials Science</td> <td>Q2</td> <td>39 / 113</td> <td>65%</td> </tr> <tr> <td></td> <td></td> <td></td> <td>Subcategory: General Dentistry</td> <td></td> <td></td> <td></td> </tr> </tbody> </table>	CiteScore	SJR	SNIP	CiteScore Rank			2.60	0.642	0.979	Subject field	Quartiles	Rank	Percentile				Category: Materials Science	Q2	49 / 106	54%				Subcategory: Ceramics and Composites							Category: Materials Science	Q2	39 / 113	65%				Subcategory: General Dentistry			
CiteScore	SJR	SNIP	CiteScore Rank																																							
2.60	0.642	0.979	Subject field	Quartiles	Rank	Percentile																																				
			Category: Materials Science	Q2	49 / 106	54%																																				
			Subcategory: Ceramics and Composites																																							
			Category: Materials Science	Q2	39 / 113	65%																																				
			Subcategory: General Dentistry																																							
Self-Citation Ratio (2019-2020)	11.00%																																									
Official Website	<a href="http://www.jstage.jst.go.jp/browse/dmj">http://www.jstage.jst.go.jp/browse/dmj</a>																																									

Chat with us 

Online Manuscript Submission	<a href="https://mc.manuscriptcentral.com/dmj">https://mc.manuscriptcentral.com/dmj</a>
Open Access	No
Publisher	JAPANESE SOC DENTAL MATERIALS DEVICES, C/O KOKU HOKEN KYOKAI, 1-43-9 KOMAGOME TS BDG, KOMAGOME, TOSHIMA-KU, TOKYO, JAPAN, 170-0003
Subject Area	Medicine
Country/Area of Publication	JAPAN
Publication Frequency	Bimonthly
Year Publication Started	1982
Annual Article Volume	129
Indexing (SCI or SCIE)	<a href="#">Science Citation Index Expanded</a>
Link to PubMed Central (PMC)	<a href="https://www.ncbi.nlm.nih.gov/nlmcatalog?term=0287-4547%5BISN%5D">https://www.ncbi.nlm.nih.gov/nlmcatalog?term=0287-4547%5BISN%5D</a>
Average Duration of Peer Review *	Authorized Data from Publisher: Data from Authors: About 3.0 month(s)
Competitiveness *	Data from Authors: Easy
Useful Links	<a href="#">Relevant Journals</a> <span style="margin-left: 200px;"><a href="#">[DENTAL MATERIALS JOURNAL] CiteScore Trend</a></span> <a href="#">Comments from Authors</a>

Chat with us 

# Dental Materials Journal

Dental Materials Journal is a peer review journal published by the Japanese Society for Dental Materials and Devices aiming to introduce the progress of the basic and applied sciences in dental [Read more](#)

Published by [The Japanese Society for Dental Materials and Devices](#)

- JOURNALS
- PEER REVIEWED
- FREE ACCESS
- ADVANCE PUBLICATION
- SCOPUS
- PUBMED

3,568 registered articles  
(updated on December 27, 2020)

Online ISSN : 1881-1361  
Print ISSN : 0287-4547  
ISSN-L : 0287-4547

1.359  
2019 Journal Impact Factor (JIF)



- Journal home
- Advance online publication
- Journal issue
- Featured articles
- About the journal

J-STAGE home / Dental Materials Journal / Journal home

## Featured article

Volume 33 (2014) Issue 5 Pages 705-710

### Mechanical properties of composite resin blocks for CAD/CAM

Sasipin LAUVAHUTANON, Hidekazu TAKAHASHI, Maho SHIOZAWA, Naohiko IWASAKI, Yuya ASAKAWA, Meiko OKI, Werner J. FINGER, Mansuwan ARKSORNNUKIT

This study compared commercial composite resin blocks with one ceramic block for use in computer-aided design/computer aided manufacturing (CAD/CAM). Four composite resins, one composite ceramic, and one feldspar-ceramic block were investigated. Flexural strength (FS), flexural modulus (FM), and Vickers hardness (VH) were determined under three conditions: dry storage, immersion in water at 37°C for 7 days, and immersion in water at 37°C for 7 days followed by 10,000

thermocycles. After dry storage, FS ranged from 127 to 242 MPa, FM from 9.6 to 51.5 GPa, and VH from 64 to 455. Two-way ANOVA was performed for FS, FM and VH followed by Tukey's multiple comparison ( $\alpha < 0.05$ ). Results demonstrated that the materials degraded after water immersion and thermocycling, but their properties

[Read more](#)

#### Editor's picks

Field Weighted Citation Impact (FWCI) is one of indices to evaluate the scientific publishing by estimating the total citation ratio based on the average of the subject field from Scopus database. FWCI could therefore be used as the index over specific field. Here, we show the example of DMJ articles from 2014 to 2016 with relatively higher FWCI values beyond 1.0 which is considered the average of the subject field. The editors of the DMJ would like to introduce some of the articles here. FWCI score of this article is 4.29.

[View all featured articles](#)

## Most viewed articles Nov.2020

- 1** Comprehensive review of current endodontic sealers  
Released: September 29, 2020 | Volume 39 Issue 5 Pages 703-720  
Takashi KOMABAYASHI, David COLMENAR, Nicholas CVACH, Aparna BHAT, Carolyn PRIMUS, Yohji IMAI  
Views: 171
- 2** A review of dental CAD/CAM: current status and future perspectives from 20 years of experience  
Released: July 10, 2009 | Volume 28 Issue 1 Pages 44-56  
Takashi MIYAZAKI, Yasuhiro HOTTA, Jun KUNII, Soichi KURIYAMA, Yukimichi TAMAKI  
Views: 160
- 3** Current status of direct pulp-capping materials for permanent teeth  
Released: January 31, 2016 | Volume 35 Issue 1 Pages 1-12  
Takashi KOMABAYASHI, Qiang ZHU, Robert EBERHART, Yohji IMAI  
Views: 146
- 4** Comprehensive review of current endodontic sealers  
Released: March 24, 2020 | Article ID 2019-288  
Takashi KOMABAYASHI, David COLMENAR, Nicholas CVACH, Aparna BHAT, Carolyn PRIMUS, Yohji IMAI  
Views: 143

feedback

feedback

feedback



## 2020 Volume 39 Issue 6

### Activation of matrix-bound endogenous proteases by self-etch adhesives

Bebek Serra OGUZ AHMET, Roda SESEOGULLARI-DIRIHAN, Arzu TEZVERGIL-MUTLUAY

### Effect of two bleaching regimens on enamel bonding performance

Somayah HALABI, Naoko MATSUI, Toru NIKAI, Ahmed ABDQ, Michael F. BURROW, Junji TAGAMI

### Influence of mucin pre-adsorption for lipoteichoic acid adsorption on titanium surfaces

Eiji YOSHIDA, Tohru HAYAKAWA

### Silicon nitride ceramic for all-ceramic dental restorations

Mahmut Sertaç ÖZDOĞAN, Mustafa GÜNGÖRMÜŞ, Ali ÇELİK, Gülsüm TOPATEŞ

[View all articles in Current issue](#)


Select past volume & issue

Volume ▾ Issue ▾ Go

[Submit your paper](#) >

[How to submit](#) >

[Information for authors](#) >

[RSS feed \(Issue\)](#) 

[RSS feed \(Article\)](#) 

Favorites & Alerts

[☆ Add to favorites](#)

[☆ Announcement alert](#)

[☆ New arrival alert](#)

## Most viewed articles Nov.2020

- 1** **Comprehensive review of current endodontic sealers**  
Released: September 29, 2020 | Volume 39 Issue 5 Pages 703-720  
Takashi KOMABAYASHI, David COLMENAR, Nicholas CVACH, Aparna BHAT, Carolyn PRIMUS, Yohji IMAI  
Views: 171
- 2** **A review of dental CAD/CAM: current status and future perspectives from 20 years of experience**  
Released: July 10, 2009 | Volume 28 Issue 1 Pages 44-56  
Takashi MIYAZAKI, Yasuhiro HOTTA, Jun KUNII, Soichi KURIYAMA, Yukimichi TAMAKI  
Views: 160
- 3** **Current status of direct pulp-capping materials for permanent teeth**  
Released: January 31, 2016 | Volume 35 Issue 1 Pages 1-12  
Takashi KOMABAYASHI, Qiang ZHU, Robert EBERHART, Yohji IMAI  
Views: 146
- 4** **Comprehensive review of current endodontic sealers**  
Released: March 24, 2020 | Article ID 2019-288  
Takashi KOMABAYASHI, David COLMENAR, Nicholas CVACH, Aparna BHAT, Carolyn PRIMUS, Yohji IMAI  
Views: 143
- 5** **Thermal Properties of Dental Materials**  
Released: February 12, 2009 | Volume 23 Issue 3 Pages 399-405  
Masahiro SAITOH, Shigeyuki MASUTANI, Taishi KOJIMA, Masataka SAIGO, Hideharu HIROSE, Minoru NISHIYAMA  
Views: 136

Share this page



feedback

feedback



feedback

# DENTAL MATERIALS JOURNAL

Volume 26,  
Number


4

July 2007

AN OFFICIAL  
JOURNAL OF

THE JAPANESE SOCIETY  
FOR DENTAL MATERIALS  
AND DEVICES

JAPAN SOCIETY FOR  
ADHESIVE DENTISTRY



The Japanese Society  
for Dental Materials and Devices  
<http://wwwsoc.nii.ac.jp/jsdmd/index-e.shtml>

# The Japanese Society for Dental Materials and Devices

## Board of Directors

<b>President:</b>	Takashi MIYAZAKI
<b>Vice-President</b> <b>and Director, Editorial Board:</b>	Susumu HIRANO
<b>Director, Secretary:</b>	Yoshima ARAKI
<b>Director, Planning:</b>	Kazuomi SUZUKI
<b>Director, Treasurer:</b>	Kunio ISHIKAWA
<b>Director, Public Relations:</b>	Tatsushi KAWAI
<b>Director, Liaison Affairs:</b>	Hidekazu TAKAHASHI
<b>Director, Education:</b>	Kozo UMEMOTO

## Editorial Board of Dental Materials Journal

<b>Editor-in-Chief:</b>	Kazuomi SUZUKI	
<b>Vice-Editor:</b>	Kunio ISHIKAWA	
<b>Vice-Editor:</b>	Hideo MATSUMURA	
<b>Editorial Board:</b>	Michael F. BURROW	Taiji SOUMURA
	San-Y. CHEN	Hidehiko SANO
	Lawrence GETTLEMAN	Yukyo TAKADA
	Shigeru HIRABAYASHI	Shoji TAKEDA
	Satoshi IMAZATO	Takuo TANAKA
	Yoshinori KADOMA	Naomi TANOUE
	Minoru KAWAGUCHI	Shozo TSURUTA
	Hyung-I. KIM	Motohiro UO
	Shigeaki KURATA	Bart VAN MEERBEEK
	Masaharu NAKAGAWA	Nobukazu WAKAMATSU
	Toru NIKAIDO	Yasuhiro YOSHIDA
	John M. POWERS	

## Address of Office

The Japanese Society for Dental Materials and Devices c/o Koku Hoken Kyokai  
1-43-9 Komagome TS Bdg., Komagome, Toshima-ku, Tokyo 170-0003, Japan  
TEL: +81-3-3947-8891 FAX: +81-3-3947-8341

Overseas Distributor (Members, Non-members)  
Japan Publication Trading Co., Ltd.  
P.O. Box 5030 Tokyo International, Tokyo, Japan

# Contents

## Original papers

### Application of Plasma Immersion Ion Implantation for Surface Modification of Nickel-titanium Rotary Instruments

Uei-Ming LI, Masahiro IJIMA, Kazuhiko ENDO, William A. BRANTLEY,  
Satish B. ALAPATI and Chun-Pin LIN ————— 467

### Priming Effects of Triethylene Glycol and Triethylene Glycol Monomethacrylate on Dentin Bonding

Mizuho KUSUNOKI, Kazuo ITOH, Yutaka UTSUMI and Hisashi HISAMITSU ————— 474

### Effects of Dose of Recombinant Human BMP-2 on Bone Formation at Palatal Sites in Young and Old Rats

Kozo YAMAJI, Masamitsu KAWANAMI, Atsushi MATSUMOTO, Tomoomi ODAJIMA,  
Yoshihiro NISHITANI, Kensuke IWASAKA, Keiko YOSHIMITSU and Masahiro YOSHIYAMA — 481

### Synthetic Osteopontin-derived Peptide SVVYGLR can Induce Neovascularization in Artificial Bone Marrow Scaffold Biomaterials

Yoshinosuke HAMADA, Hiroshi EGUSA, Yoshitoshi KANEDA, Isao HIRATA,  
Naomasa KAWAGUCHI, Takafumi HIRAO, Takuya MATSUMOTO, Makiko YAO,  
Kiyoshi DAITO, Mayuka SUZUKI, Hirofumi YATANI, Michiharu DAITO,  
Masayuki OKAZAKI and Nariaki MATSUURA ————— 487

### Hardness and Elasticity of Sound and Caries-affected Primary Dentin Bonded with One-step Self-etch Adhesive

Yumiko HOSOYA, Franklin R. TAY, Masashi MIYAZAKI and Takashi INOUE ————— 493

### Effects of Monomer Composition and Original Filler Content on Filler Loading in the Resulting Centrifuged Composites

Naomi TANOUE, Atsushi MIKAMI, Mitsuru ATSUTA and Hideo MATSUMURA ————— 501

### Effect of Resin Coating on Dentin Bonding of Resin Cement in Class II Cavities

Shamim SULTANA, Toru NIKAIDO, Khairul MATIN, Miwako OGATA,  
Richard M. FOXTON and Junji TAGAMI ————— 506

### Surface Treatment with *N,N'*-Dimethacryloylcystine for Enhanced Bonding of Resin to Dental Alloys

Jiro TANAKA, Jeffrey W. STANSBURY, Joseph M. ANTONUCCI and Kazuomi SUZUKI ————— 514

### Enhancement of Adhesion between Resin Coating Materials and Resin Cements

Tomoaki UDO, Toru NIKAIDO, Masaomi IKEDA, Dinesh S WEERASINGHE, Naoko HARADA,  
Richard M. FOXTON and Junji TAGAMI ————— 519

### Mechanical Behavior of Glass Ionomer Cements as a Function of Loading Condition and Mixing Procedure

Nicoleta ILIE and Reinhard HICKEL ————— 526

### Stress Analysis of Clasps Made of Glass Fiber-reinforced Composite Material Using Three-dimensional Finite Element Method : Influence of Shape in Cross and Longitudinal Sections of Circumferential Clasp Arms

Hiromi MARUYAMA, Tohru HAMANO, Chie KISHITA, Yasuhiro NISHI,  
Shinichiro KAWAMOTO and Eiichi NAGAOKA ————— 534

<b>Effects of Mica and Glass on Surface Hardness of Acrylic Tooth Material</b> Fatma UNALAN and Idil DIKBAS	545
<b>Machining Accuracy of Crowns by CAD/CAM System Using TCP/IP : Influence of Restorative Material and Scanning Condition</b> Sachiko TOMITA, Akiyoshi SHIN-YA, Harunori GOMI, Akikazu SHIN-YA and Daiichiro YOKOYAMA	549
<b>A Numerical Simulation of Orthodontic Tooth Movement Produced by a Canine Retraction Spring</b> Yukio KOJIMA, Toshihiro MIZUNO, Sachio UMEMURA and Hisao FUKUI	561
<b>Immobilization of Simulated Reducing Agent at the Surface of SiO<sub>2</sub> Fillers in Dental Composite Resins</b> Satoki SHIBATA, Isao HIRATA, Yuji NOMURA, Kenichi SHIRAI, Morioki FUJITANI, Hideaki SHINTANI and Masayuki OKAZAKI	568
<b>Influence of Light Irradiation Condition on Microshear Bond Strength of Dual-cured Resin Luting Agents</b> Xiangfeng MENG, Keiichi YOSHIDA and Mitsuru ATSUTA	575
<b>Resin Infiltration of Artificial Enamel Caries Lesions with Experimental Light Curing Resins</b> Sebastian PARIS, Hendrik MEYER-LUECKEL, Helmut CÖLFEN and Andrej M. KIELBASSA	582
<b>Technical reports</b>	
<b>Twenty-four Hour Flexural and Shear Bond Strengths of Flowable Light-cured Composites: A comparison Analysis Using Weibull Statistics</b> Rosalina TJANDRAWINATA, Masao IRIE and Kazuomi SUZUKI	589
<b>Analysis of Internal Defects in All-ceramic Crowns Using Micro-focus X-ray Computed Tomography</b> Takashi NAKAMURA, Kazumichi WAKABAYASHI, Yoshiko KAWAMURA, Soichiro KINUTA, Yoshihiko MUTOBE and Hirofumi YATANI	598
<b>Clinical Evaluation and Interfacial Morphology Observation of Xeno III Self-etching Resin Bonding and Restorative System</b> Jumpei SUGIZAKI, Makoto MORIGAMI, Shigeru UNO and Toshimoto YAMADA	602

## Twenty-four Hour Flexural and Shear Bond Strengths of Flowable Light-cured Composites: A comparison Analysis Using Weibull Statistics

Rosalina TJANDRAWINATA<sup>1</sup>, Masao IRIE<sup>2</sup> and Kazuomi SUZUKI<sup>2,3</sup>

<sup>1</sup>Department of Dental Materials, Faculty of Dentistry, Trisakti University, Campus B, Jl. Kyai Tapa 260, Jakarta 11440, Indonesia

<sup>2</sup>Department of Biomaterials, Okayama University Graduate School of Medicine, Dentistry and Pharmaceutical Science, 2-5-1, Shikata-cho, Okayama 700-8525, Japan

<sup>3</sup>Research Center for Biomedical Engineering, Okayama University, 2-5-1, Shikata-cho, Okayama 700-8525, Japan

Corresponding author, Masao IRIE; E-mail: mirie@md.okayama-u.ac.jp

Received January 25, 2007/Accepted February 26, 2007

By means of Weibull analysis, this study evaluated and compared the flexural strength and shear bond strength of flowable light-cured composites against those of conventional ones. Twenty specimens of each material were prepared for flexural and shear bond strength measurements. Specimens were measured after water storage at 37°C for 24 hours. Three of four flowable composites showed significantly higher flexural strength than conventional ones, with Weibull moduli ranging between 6 and 14. With the presence of a bonding agent, the shear bond strength to enamel of both types was not different significantly ( $p=0.28$ ), with Weibull moduli ranging between 4 and 9. In the selection of an excellent resin composite material, results of this study showed that a high, stable Weibull modulus value could be a sound indicator.

Keywords: Flowable composites, Mechanical strength, Weibull analysis

### INTRODUCTION

Presently, resin composites have replaced amalgam as the universal restorative material. Following the success of conventional composites (CCRs), demand — in tandem with continuous research development — led some manufacturers to launch flowable composites (FCRs). As such, the first generation of FCRs was introduced in late 1996, just before condensable composites<sup>1</sup>.

FCRs are materials of low viscosity. Hence, they flow easily into all the nooks and crannies, adapt readily to the tooth structure, and are able to fill irregular, internal surfaces. By virtue of these advantages, a prominent application of FCRs is inevitably as liners in areas of difficult access, such as the gingival margin of Class II preparations. The conventional wisdom is that the use of flowable composites would result in less microleakage, internal voids, and postoperative sensitivity<sup>1,2</sup>.

To date, FCRs have been explored and evaluated in numerous experiments — including as a base material in indirect Class II composite restorations<sup>3</sup>. In terms of the occurrence rate of enamel microcracks in restored teeth, it was lower with FCRs than with conventional hybrid composites<sup>4</sup>. As for Class IV restorations, FCRs were perceived as an inexpedient choice because they were acceptable only as filling materials in low-stress applications<sup>1</sup>. With due consideration to the strengths and weaknesses of FCRs, most dentists would unreservedly use FCR as a lining material while completely reserved in using FCR as a restorative material. On the other hand, other dentists would use FCRs for a wide plethora of

applications — as liners and pit and fissure sealants to repair marginal cracks and voids, as well as for Class I and V restorations<sup>5</sup>.

Fractures in the body and at the margins of restorations can lead to the failure of composite fillings. To prevent such fractures and failures, clinical studies would be the best and most effective means to characterize composite filling materials. However, clinical trials are more expensive and time-consuming than laboratory tests. Against this background, an *in vitro* determination of material parameters — such as flexural strength and shear bond strength — is a very important and helpful means of predicting clinical performance<sup>6,7</sup>.

Flexural strength measurement determines the real strength of a restorative material *per se*, while shear bond strength represents the strength of the material in correlation with tooth structure with the presence of a bonding agent. In both cases, Weibull statistical analysis is recommended because it allows for skewed data — predicting values within and outside the data set, thereby giving an “overall” analysis of the performance of a material<sup>7,12</sup>. However, no reports are available that directly compare the mechanical properties of FCRs against their CCR counterparts of a similar brand using the Weibull statistical approach. In characterizing the performance of FCRs, it is very important that they be compared directly against CCRs of a similar or same brand, so as to have a more meaningful and comprehensive understanding of their mechanical characteristics.

Polymerization is in progress even after light curing<sup>13</sup>. As such, this investigation was carried out

after 24-hour water storage to evaluate the following properties: (a) flexural strength; (b) shear bond strength; and (c) Weibull modulus. The hypothesis was that the (a), (b), and (c) properties of FCRs were correlated to each other and would be significantly different compared with the CCRs.

## MATERIALS AND METHODS

Four FCRs (Metafil Flo, Filtek Flow, Point 4 Flowable and Unifil Flow) and four CCRs (Metafil C, Filtek A110, Point 4, and Unifil F) of Shade A3, paired from the same manufacturers, were used in this study. Details of the materials used are listed in Table 1. Then, as listed in Table 2, bonding agents were chosen from the same manufacturers.

A visible light curing unit (New Light VL-II, GC; irradiated diameter: 10 mm) was used for activating the specimens, and close contact was ensured between exit window of the lamp and matrix. Before each application, light intensity was checked using a radiometer (Demetron, Kerr). During the experiment, light intensity was maintained at 450 mW/cm<sup>2</sup>.

All procedures, except for mechanical testing, were performed in a thermohygrostatic room maintained at 23 ± 0.5 and 50 ± 2 % relative humidity.

### Flexural strength test

Teflon molds of 2.0 mm depth, 2.0 mm width, and

25.0 mm length were used to fabricate specimens for flexural strength measurement.

Twenty specimens were prepared for each material. Each mold was filled with the material, covered with a celluloid strip and a glass plate, then clamped. After 15 seconds, the glass plate was removed and the specimen light-cured in three sections with an overlap of 2 mm and an irradiation time of 20, 30, or 40 seconds according to manufacturer's recommendations. After light curing, the material was removed from the mold while excess filling material was removed with a silicon carbide bur. Then, the specimens were polished with a wet sandpaper (#600) to achieve a flat, even surface. After immersion in distilled water in a 37 °C incubator for 24 hours, the specimens were measured using a digital micrometer (No. 293 - 421 - 20, Mitutoyo) and tested.

Flexural strength was measured using the three-point bending method with a 20-mm span at a crosshead speed of 0.5 mm/min, by mounting the apparatus on a universal testing machine (Autograph DCS-2000, Shimadzu) as outlined in ISO 4049. A maximum external force of 10 kgf (98 N) was applied to the midpoint of test beam. Then, the stress at failure was calculated and recorded as the flexural strength of each material<sup>16,12,13</sup>.

### Shear bond strength test to enamel

Random samples of human premolar teeth, extracted

Table 1 Materials investigated in this study. Information as provided by the manufacturers

Material	Manufacturer	Batch no.	Filler	Monomer	Curing time(s)
Metafil Flo* (microfilled)	Sun Medical, Mori-yama, Japan	VV10, VV12, EK1, EK2	Barium silica glass, colloidal silica, and TMPT Filler content: 44 vol% (65 wt%) Filler particle size: 0.01 - 10 μm	UDMA	40
Metafil C** (microfilled)	Sun Medical, Mori-yama, Japan	TE1	TMPT and colloidal silica Filler content: 54 vol% (66 wt%) Filler particle size: 0.01 - 10 μm	UDMA	40
Filtek™ Flow* (microfilled)	3M, St. Paul, MN, USA	OBK, 20010104	Silica and silica zirconia Filler content: 47 vol% (68 wt%) Filler particle size: 1.50 μm	Bis-GMA, TEGDMA	20
Filtek A110** (microfilled)	3M, St. Paul, MN, USA	1AP	Inorganic silica Filler content: 40 vol% (56 wt%) Filler particle size: 0.04 μm	Bis-GMA	40
Point 4 Flowable* (microhybrid)	Kerr, Orange, CA, USA	206B43	Barium silica glass Filler content: 48 vol% (70 wt%)	TEGDMA, EBPADM	40
Point 4** (microhybrid)	Kerr, Orange, CA, USA	205553	Barium aluminoborosilicate glass Filler content: 57 vol% (76 wt%) Filler particle size: 0.4 μm	BISGMA, TEGDMA, EBPADM	40
Unifil Flow* (microhybrid)	GC Corp., Tokyo, Japan	0107201	Fluoroaluminosilicate glass, silica Filler content: 67 wt% (vol%: not Available) Filler particle size: 0.7 μm	UDMA (26%) Dimethacrylate (7%)	40
Unifil F** (microhybrid)	GC Corp., Tokyo, Japan	161181, 0204031	Fluoroaluminosilicate glass, silica Filler content: 77 wt% (vol%: not Available) Filler particle size: 0.8 - 0.9 μm	UDMA (16%) Dimethacrylate (7%)	20

\*: Flowable type (FCR); \*\*: Conventional type (CCR); Bis-GMA: Bisphenol A diglycidylmethacrylate; EBPADM: Ethoxylated bisphenol A dimethacrylate; TEGDMA: Triethylene glycol dimethacrylate; TMPT: Trimethylol ropane trimethacrylate; UDMA: Urethane dimethacrylate

Table 2 Bonding agents used in this study. Information as provided by the manufacturers

Bonding product	Manufacturer	Batch no.	Restorative material	Components and procedure
AQ Bond	Sun Medical, Moriyama, Japan	FF1	Metafil Flo, Metafil C	One-bottle bonding agent: 4-META AQ sponge: bonding promoter AQ sponge + bond, coat 20 s, air-blow 3 - 5 s, 2 <sup>nd</sup> coat, air blow 5 - 10 s, light cure 10 s.
Single Bond	3M, St. Paul, MN, USA	20020603	Filtek Flow, Filtek A110	Etchant: 35% H <sub>3</sub> PO <sub>4</sub> Primer and adhesive: H <sub>2</sub> O, ethanol, HEMA, BisGMA, dimethacrylates, polyalkenoic acid copolymer, photoinitiator Etching 15 s, rinse 10 s, air-blow 1 s, adhesive 2 times, air-blow 2 - 5 s, light cure 10 s.
OptiBond Solo	Kerr, Orange, CA, USA	110B16	Point 4 Flowable, Point 4	Etchant: 37.5% H <sub>3</sub> PO <sub>4</sub> Primer and adhesive: BHT, CQ, EtOH, HEMA, GPDM, fumed silica, NaSiF, barium aluminoborosilicate, BisGMA, ODMAB Etching 15 s, rinse 10 s, air blow 1 s, adhesive 15 s, air blow 3 s, light cure 20 s.
Unifil Bond	GC Corp., Tokyo, Japan	0206101	Unifil Flow, Unifil F	Monomer: carbonic acid, HEMA Self-etching primer 20 s, air blow 5 s, bonding agent, light cure 10 s.

BHT: 2,6-Di-tert-butyl-4-methylphenol (inhibitor); BisGMA: Bisphenol A diglycidylmethacrylate; CQ: Camphorquinone; EtOH: Ethanol; GPDM: Glycerol phosphate dimethacrylate; H<sub>3</sub>PO<sub>4</sub>: Phosphoric acid; HEMA: Hydroxyethyl methacrylate; NaSiF: Sodium hexafluorosilicate; ODMAB: 2-ethylhexyl 4-dimethylamino benzoate

for orthodontic reasons, were used to measure the shear bond strength to enamel. After extraction and cleaning, the teeth were stored immediately in distilled water at about 4 °C within three months before use. Flat, proximal enamel surfaces were used in this study. The teeth were embedded in a slow-setting epoxy resin (Epofix Resin, Struers) in cylindrical rubber molds (25 mm in diameter), with the proximal site for bonding facing the bottom of the mold. Embedded specimens were ground flat on a wet SiC abrasive paper up to 1000-grit, until an area of at least 4 mm in diameter was exposed in enamel.

A split Teflon mold with a cylindrical hole (diameter of 3.6 mm; height of 2.0 mm) was clamped to the prepared enamel surface. Etching and bonding agents were applied to the enamel surface according to manufacturers' instructions. The bonding materials used in this study are listed in Table 2. The Teflon mold was filled with the restorative material, covered with a celluloid strip and a glass plate, then clamped. After 15 seconds, the glass plate was removed. Then, the specimen was light-cured with an irradiation time of 20, 30, or 40 seconds according to manufacturer's recommendations before it was removed from the mold.

Of each material, 20 specimens were prepared. The prepared specimens were immersed in distilled water in a 37 °C incubator. After 24 hours, they were measured using a digital micrometer and then secured in a mounting jig. Shear force was transmitted by a flat, blunt, 1-mm-broad shearing edge at a 90 ° angle to the direction of the load and at the back of the loading plate. Shear bond strength test

was conducted using a universal testing machine, where shear force was applied at a crosshead speed of 0.5 mm/min with a maximum external force of 50 kgf (490 N). Stress at failure was calculated and recorded as the shear bond strength<sup>14</sup>.

After shear bond strength measurement, fracture surfaces of the samples were ultrasonically washed in distilled water for two minutes and then lightly air-dried. To prepare for examination using a field emission scanning electron microscope (FE-SEM; DS-720, Topcon), the surfaces were coated with gold (Ion Coater IB-3, Eiko Engineering Co. Ltd.) at 7 mA for 240 seconds. Representative areas of test sites were photographed at ×1000 magnification.

#### Statistical analysis

Results of flexural and shear bond strength measurements were analyzed using Weibull statistics with the following equation:

$$Pf = 1 - \exp[-(s/\sigma)^m]$$

where  $Pf$  is the probability of failure,  $s$  is the strength at a given  $Pf$ ,  $\sigma$  is the characteristic strength, and  $m$  is the Weibull modulus a constant factor related to the dispersion of failure strength data<sup>8,9</sup>.

All measurements were also analyzed using one-way ANOVA and Tukey's test. Strengths between pairs were distinguished using t-test<sup>15</sup>. Possible correlations between parameters were analyzed using a SigmaPlot 8.0 program (SPSS, Chicago, Illinois, USA).

RESULTS

*Flexural strength test*

Table 3 lists the Weibull analysis of the 24-hour flexural strength values. All FCRs, except Point 4 Flowable, showed a higher 24-hour flexural strength

value than their CCR counterparts. Further, all composite pairs showed significant differences between the mean values of FCR and CCR, except with the Unifil pair. The mean flexural strength value of Metafil Flo was 1.3-fold of Metafil C, that of Filtek™ Flow was 1.9-fold of Filtek A110, and that

Table 3 Weibull analysis of 24-hour flexural strengths

Material	Mean (SD) <sup>#</sup> (MPa)	Characteristic strength (σ <sub>0</sub> ) (MPa)	Weibull modulus (m)	Correlation coefficient (r)	Stress for 10% chance of failure σ <sub>0.10</sub> (MPa)	Stress for 90% chance of failure σ <sub>0.90</sub> (MPa)
Metafil Flo*	128.1 (13.6) <sup>b,c</sup>	134.5	9.68	0.97	106.6	146.6
Metafil C**	98.0 (8.4) <sup>e</sup>	101.9	12.39	0.97	85.0	109.0
Filtek™ Flow*	133.1 (9.7) <sup>a,b</sup>	137.7	14.30	0.96	117.7	146.0
Filtek A110**	71.1 (6.5) <sup>f</sup>	74.2	11.20	0.97	60.7	80.0
Point 4 Flowable*	100.7 (14.6) <sup>e</sup>	107.1	7.31	0.97	78.7	120.1
Point 4**	141.4 (15.6) <sup>a</sup>	148.5	9.52	0.95	117.3	162.1
Unifil Flow*	118.4 (13.1) <sup>c,d</sup>	124.8	8.84	0.97	96.7	137.1
Unifil F**	109.1 (18.5) <sup>d,e</sup>	117.1	6.17	0.99	81.3	134.0

n=20; \*: Flowable light-cured composite resin; \*\*: Conventional light-cured composite resin; #: Identical letters indicate no significant differences according to Tukey's test (p>0.05).

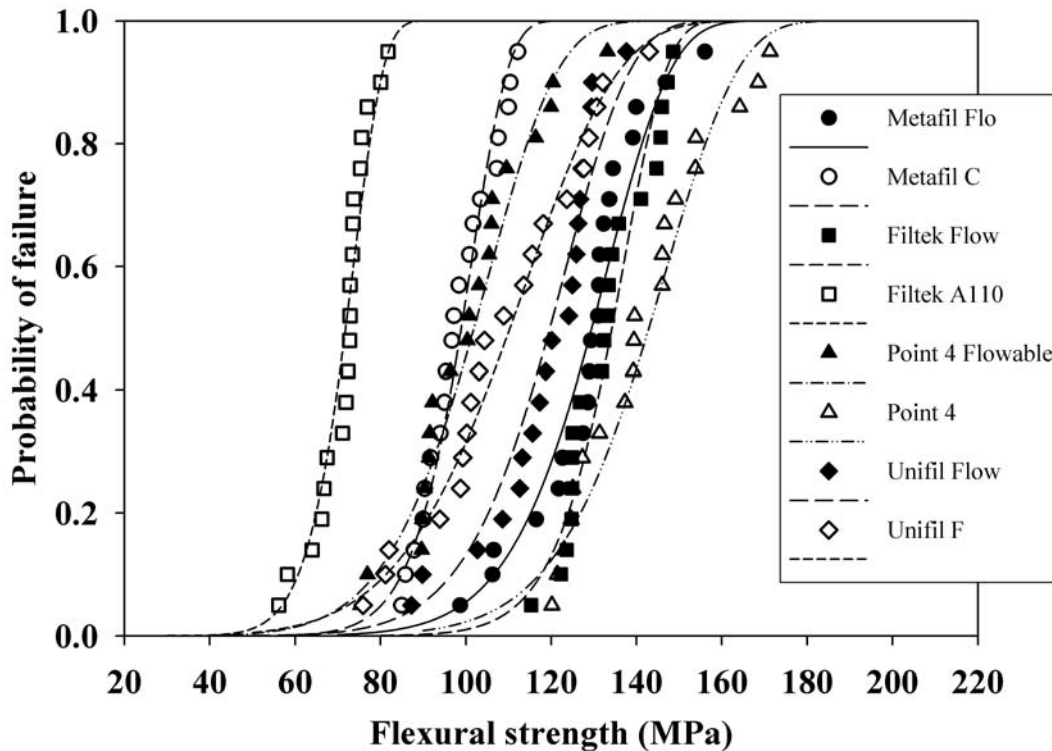


Fig. 1 Weibull distribution analysis of flexural strength data. Lines indicate the fitting curves of  $P_f = 1 - \exp[-(\sigma / \sigma_0)^m]$ .

Table 4 Weibull analysis of 24-hour shear bond strengths to enamel

Material	Mean (SD)# (MPa)	Characteristic strength (σ) (MPa)	Weibull modulus (m)	Correlation coefficient (r)	Stress for 10% chance of failure <sub>0.10</sub> (MPa)	Stress for 90% chance of failure <sub>0.90</sub> (MPa)
Metafil Flo*	15.5 (1.5) <sup>c</sup>	13.6	4.09	0.98	7.8	16.7
Metafil C**	15.8 (1.2) <sup>c</sup>	14.3	5.81	0.98	9.7	16.5
Filtek™ Flow*	24.1 (4.0) <sup>a,b</sup>	25.8	6.31	0.97	18.1	29.5
Filtek A110**	23.5 (4.3) <sup>a,b</sup>	25.3	5.77	0.99	17.1	29.2
Point 4 Flowable*	25.9 (3.9) <sup>a</sup>	27.6	7.05	0.99	20.1	31.1
Point 4**	27.7 (3.2) <sup>a</sup>	29.2	9.17	0.99	22.8	31.9
Unifil Flow*	16.7 (4.4) <sup>c</sup>	18.4	4.11	0.97	10.6	22.5
Unifil F**	18.2 (4.8) <sup>b,c</sup>	20.0	4.02	0.99	11.4	24.6

n=20; \*: Flowable light-cured composite resin; \*\*: Conventional light-cured composite resin; #: Identical letters indicate no significant differences according to Tukey's test (p>0.05).

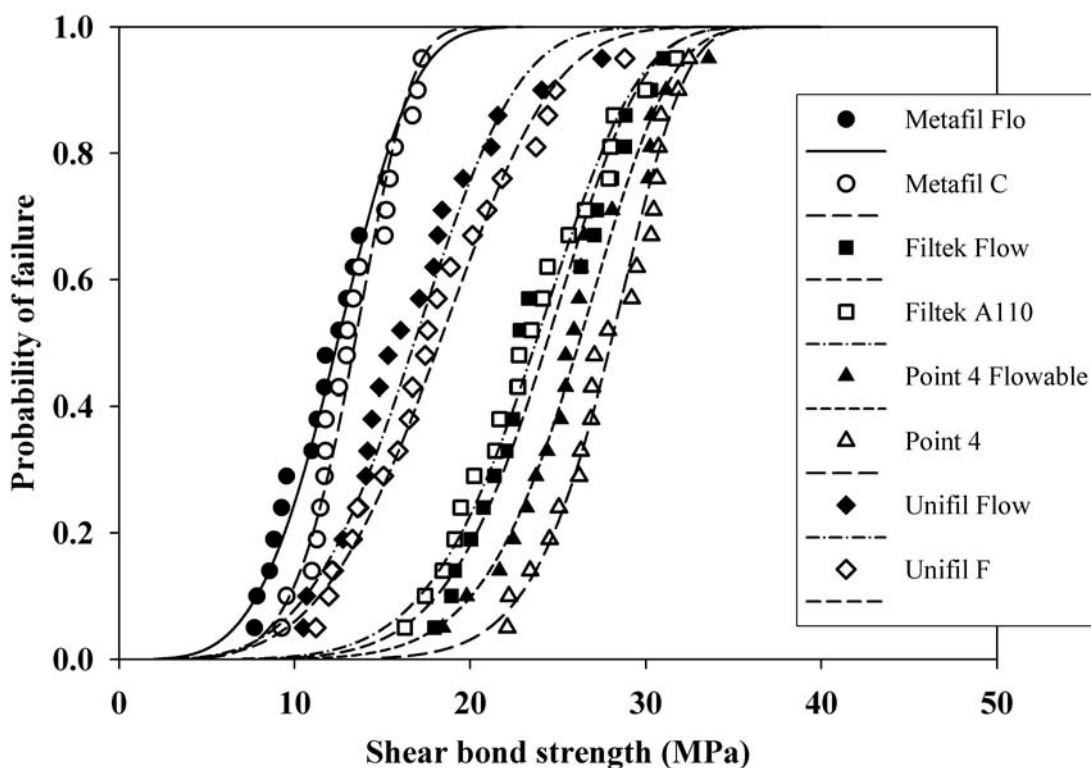


Fig. 2 Weibull distribution analysis of shear bond strength data. Lines indicate the fitting curves of  $Pf = 1 - \exp[-(\sigma / \sigma_0)^m]$ .

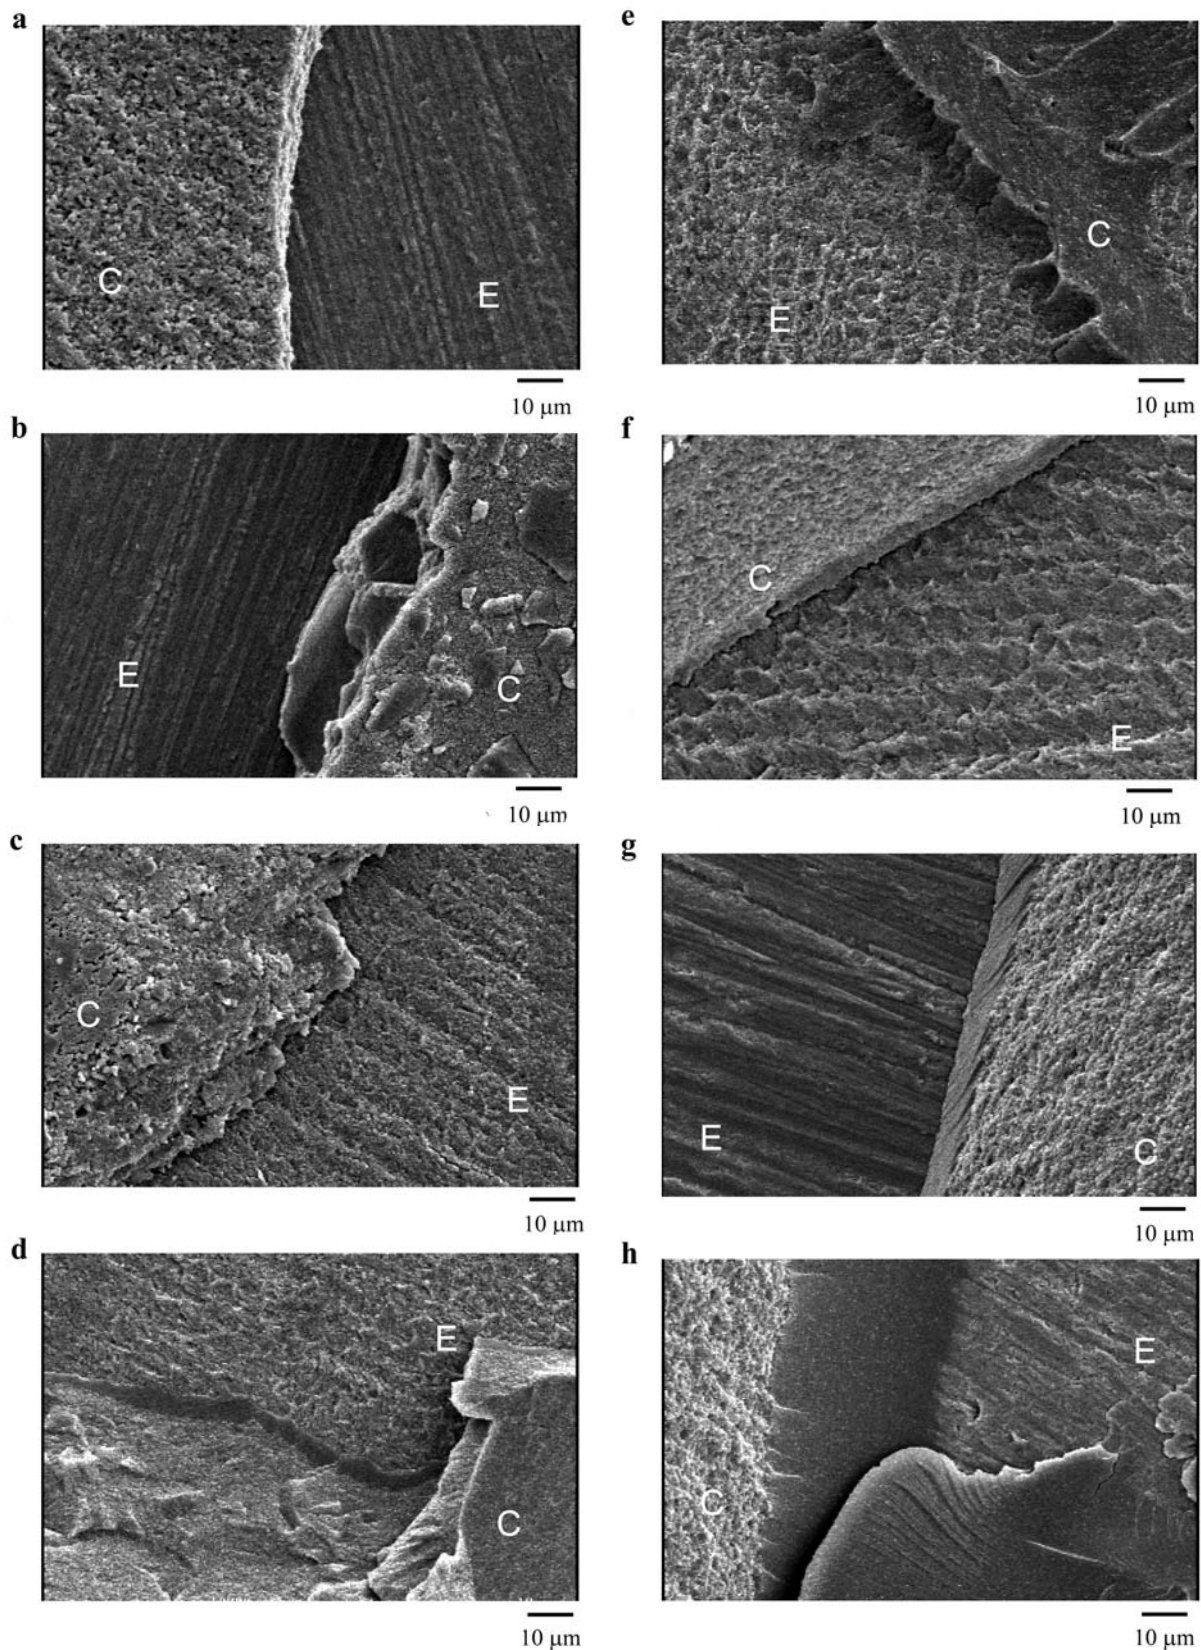


Fig. 3 Fracture modes of the specimens. C = Composite resin, E = Enamel. a: Metafil Flo, b: Metafil C, c: Filtek Flow, d: Filtek A110, e: Point 4 Flowable, f: Point 4, g: Unifil Flow, h: Unifil F.

of Unifil Flow was 1.1-fold of Unifil F. However, the mean flexural strength value of Point 4 Flowable was lower than that of Point 4 (0.7-fold).

Apart from the mean flexural strength values, Weibull analysis further showed that Point 4 had the highest characteristic strength (148.5 MPa), while Filtek A110 had the lowest characteristic strength (74.2 MPa). The Weibull moduli of materials were in the range of 6 - 14, and the correlation coefficients were in the range of 0.95 - 0.99. The Weibull curves for flexural strength are presented in Fig. 1.

#### *Shear bond strength test to enamel*

Table 4 lists the 24-hour shear bond strength values of the composites to enamel. The shear bond strengths of FCRs did not significantly differ from those of their CCR counterparts.

By means of Weibull analysis, Point 4 demonstrated the highest characteristic strength (29.2 MPa) while Metafil Flo showed the lowest (13.6 MPa). The Weibull moduli of materials were in the range of 4 - 9, and the correlation coefficients were in the range of 0.97 - 0.99. The Weibull curves for shear bond strength are presented in Fig. 2.

Figure 3 shows the SEM images of the fracture surfaces. All materials showed a mixed fracture mode, as indicated by the retention of composite resin on the enamel surfaces.

#### *Statistical analysis*

Application of t-test to each pair produced significant differences in flexural strength ( $p < 0.001$ ). However, for shear bond strength, each pair showed no significant differences (P4 pairs,  $p = 0.11$ ; Metafil pairs,  $p = 0.30$ ; Filtek pairs,  $p = 0.64$ ; and Unifil pairs,  $p = 0.33$ ). The analysis of possible correlations between flexural and shear bond strength values ( $r^2 = 0.0003$ ) and between the Weibull moduli of flexural and shear bond strengths ( $r^2 = 0.1801$ ) gave no significant correlation ( $p > 0.05$ ).

## DISCUSSION

Results of flexural strength measurement of the present study agreed with those of previous studies whereby Weibull moduli ranged between 6 and 9 for composite resins<sup>16</sup>, and between 8.52 and 14.19 for FCRs<sup>12</sup>. As for the Weibull moduli of FCRs and CCRs in the present study, there seemed to be no clear significant difference pattern between them. In terms of flexural strength, there were significant differences between FCRs and CCRs. However, for shear bond strength, there were no significant differences between the pairs, as further indicated by the Weibull moduli.

In the fractured specimens of all composites, Fig. 3 showed that some composite resin was retained on

all enamel surfaces. These SEM images clearly showed that the application of bonding agent on tooth substrate played an important role in influencing shear bond strength. At this juncture, it must be highlighted that the HEMA content which enhances monomer diffusion in dentin substrates<sup>17,18</sup> in the composition of Single Bond, Optibond Solo, and Unifil Bond did not show particular effect on shear bond strength to enamel. In contrast, a total etching procedure with phosphoric acid before applying Single Bond or Optibond Solo significantly resulted in an obvious pattern of enamel prisms on the fracture surfaces, which was not shown in the other two pairs. This etching procedure might also be a reason for the higher shear bond strengths of both Filtek and Point 4 pairs, despite the low flexural strength value of Filtek A110.

In agreement with another previous study<sup>19</sup>, the shear bond strength values were lower than the flexural strength values. Compared to a previous study on tensile bond strength<sup>7</sup>, the results of this study also showed a similar tendency, *i.e.*, disparity between bond strength and mechanical properties of composite resins. In that study<sup>7</sup>, it was shown that the tensile strengths of restorative resins bonded to dentin, and the resultant dentin bond strengths between the two, exhibited wide variability. In particular, the tensile strengths of the restorative resins gave higher Weibull moduli. This great disparity in tensile strength and bond strength results, as revealed by Weibull probability of failure method, was attributed to the multiple variables at play during tensile and bond strength tests such as specimen preparation and storage, test rig design, experimental technique, and even the brittle nature of the restorative materials.

In a study which used a shear punch test<sup>10</sup>, the Weibull modulus range obtained was 4 - 10 which was also similar to the range of 5 - 10 obtained for shear bond strength in this study. Nonetheless, on the overall, most of the values were lower than 6 a result range attributed to the application of bonding agent on the tooth surface. It could thus be said that the shear bond strength results in this study were quite reliable, when compared with adhesive bonding data that typically produce Weibull modulus values in the range of 1 - 4 or 1 - 5<sup>7,20</sup>. As for flexural strength, most composite resins showed Weibull modulus values which were 1.5 - 2.4-folds that of shear bond strength. However, two materials showed similar Weibull moduli for flexural strength and shear bond strength: Point 4 Flowable with  $m = 7$  and Point 4 with  $m = 9$ . It was thought that the EBPADM/TEGDMA content in Point 4 pair, which renders greater toughness and degree of conversion to the composites<sup>21</sup>, has played an important role. In the same vein, therefore, factors that may influence

the Weibull modulus values of shear bond strength such as chemical bonding efficacy to tooth tissues and influence of bonding agents and composite resins should be further investigated and evaluated in future experiments.

McCabe *et al.* stated that a Weibull modulus value of at least 10 is necessary for a test to be acceptable for multicenter testing<sup>22)</sup>. In view of the Weibull modulus values presented here, it seemed that the shear bond strength test performed in this study did not meet this criterion. Therefore, to be valid for multicenter testing, it is of utmost importance that the test method is selected after careful consideration of conditions that may affect test results.

For the purpose of clinical use, the most straightforward indicator would be a Weibull modulus with the highest value<sup>7,23)</sup>. In this study, however, we counter-proposed stable values as those shown by Point 4 pair to be used instead as a valid indicator for excellent composite restoratives. Furthermore, their favorable flexural strength and shear bond strength values augured well for clinical application. With reference to the data interpretation approach adopted in this study, we recommended that experimental data should be interpreted carefully and discerningly, paying particular attention to the trends and tendencies of Weibull distributions. This is because Weibull analysis not only can identify the characteristic strength for a spread of data, but also the stress level that a dental material should meet if not exceed in order to be accepted as an excellent material.

Many cases of clinical failure occur stemming from the 10% - 20% chance of failure<sup>9,20)</sup>. Failures in such circumstances are unlikely to be predicted by mere consideration of the mean value of any mechanical property. However, with Weibull analysis, the strength of 10% probability of fracture ( $\sigma_{0.10}$ ) was also determined without considering the mean value. In other words, Weibull statistics is a technique that can also be used to predict the probability of failure of dental restorative materials at any level of flexural stress application<sup>9)</sup>. In addition, the values of  $\sigma_{0.90}$  the stress level at which one would expect a 90% chance of fracture could also be analyzed to predict the upper limit of strength<sup>12)</sup>.

The Weibull cumulative plots (Figs. 1 and 2) show the failure prediction for all FCRs and CCRs. Compared to their CCR counterparts, almost all FCRs showed higher 24-hour flexural strength values. The weakest link in composites appeared to be the interface between the filler particles and resin matrix. As the filler contents of FCRs were lower than those of CCRs, it thus seemed reasonable that cracks occurred more readily in CCRs than in FCRs. Moreover, besides monomer type, filler content, filler

particle size, interparticle spacing, and coupling agent, water influences the strength of restorative materials by affecting the filler-matrix interface<sup>19,23,24)</sup>. Nonetheless, with FCRs, water sorption which is accompanied by hygroscopic expansion will help to compensate the effects of polymerization shrinkage.

## CONCLUSIONS

Flowable composites were found to have higher 24-hour flexural strengths than the conventional ones. However, the shear bond strength to tooth enamel of flowable and conventional composites were similar, due to the application of a bonding agent. In the selection of an excellent resin composite material, results of this study showed that a high, stable Weibull modulus value could be a sound indicator.

## ACKNOWLEDGEMENTS

The authors wish to thank the manufacturers for their generous donation of materials for this research project.

## REFERENCES

- 1) Bayne SC, Thompson JY, Swift EJ, Stamatides P, Wilkerson M. A characterization of first-generation flowable composite. *J Am Dent Assoc* 1998; 129: 567-577.
- 2) Chuang SF, Liu JK, Jin YT. Microleakage and internal voids in Class II composite restorations with flowable composite linings. *Oper Dent* 2001; 26: 193-200.
- 3) Dietschi D, Olsburgh S, Krejci I, Davidson C. *In vitro* evaluation of marginal and internal adaptation after occlusal stressing of indirect class II composite restorations with different resinous bases. *Eur J Oral Sci* 2003; 111: 73-80.
- 4) Han L, Okamoto A, Fukushima M, Okiji T. Enamel micro-cracks produced around restorations with flowable composites. *Dent Mater J* 2005; 24: 83-91.
- 5) Attar N, Tam LE, McComb D. Flow, strength, stiffness and radiopacity of flowable resin composites. *J Can Dent Assoc* 2003; 69: 516-521.
- 6) Anusavice KJ. *Phillips' science of dental materials*, 11<sup>th</sup> ed, Saunders-Elsevier Science, St Louis, 2003, pp.78-90, 400-430.
- 7) Burrow MF, Thomas D, Swain MV, Tyas MJ. Analysis of tensile bond strengths using Weibull statistics. *Biomaterials* 2004; 25: 5031-5035.
- 8) Weibull WA. A statistical distribution function of wide applicability. *J Appl Mech* 1951; 18: 293-297.
- 9) McCabe JF, Carrick TE. A statistical approach to the mechanical testing of dental materials. *Dent Mater* 1986; 2: 139-142.
- 10) Nomoto R, Carrick TE, McCabe JF. Suitability of a shear punch test for dental restorative materials. *Dent Mater* 2001; 17: 415-421.
- 11) Hobson RS, McCabe JF. Relationship between enamel etch characteristics and resin-enamel bond strength. *Brit Dent J* 2002; 192: 463-468.

- 12) Tjandrawinata R, Irie M, Suzuki K. Flexural properties of eight flowable light-cured restorative materials, in immediate vs. 24-hour water storage. *Oper Dent* 2005; 30: 239-249.
- 13) Cesar PF, Miranda Junior WG, Braga RR. Influence of shade and storage time on the flexural strength, flexural modulus and hardness of composites used for indirect restorations. *J Prosthet Dent* 2001; 86: 289-296.
- 14) Tjandrawinata R, Irie M, Suzuki K. Marginal gap formation and fluoride release of resin-modified glass-ionomer cement: effect of silanized spherical silica filler addition. *Dent Mater J* 2004; 23: 305-313.
- 15) Stansbury JW. Synthesis and evaluation of novel multifunctional oligomers for dentistry. *J Dent Res* 1992;
- 16) Palin WM, Fleming GJP, Burke FJT, Marquis PM, Randall RC. The reliability in flexural strength testing of a novel dental composite. *J Dent* 2003; 31: 549-557.
- 17) Nakabayashi N, Takarada K. Effect of HEMA on bonding to dentin. *Dent Mater* 1992; 8: 125-130
- 18) Xu J, Stangel I, Butler IS, Gilson DFR. An FT-Raman Spectroscopic investigation of dentin and collagen surfaces modified by 2-hydroxyethylmethacrylate. *J Dent Res* 1997; 76: 596-601.
- 19) Baran GR, Cool JI, Paul D, Boberick K, Wunder S. Weibull models of fracture strengths and fatigue behavior of dental resins in flexure and shear. *J Biomed Mater Res (App; Biomater)* 1998; 43: 226-233.
- 20) McCabe JF, Walls AWG. The treatment of results for tensile bond strength testing. *J Dent* 1986; 14: 165-168.
- 21) Stansbury JW. Synthesis and evaluation of novel multifunctional oligomers for dentistry. *J Dent Res* 1992; 71: 434-437.
- 22) McCabe JF, Watts DC, Wilson HJ, Worthington HV. An investigation of dental materials and the statistical treatment of results. *J Dent* 1990; 18: 90-97.
- 23) Manhart J, Kunzelmann KH, Chen HT, Hickel R. Mechanical properties and wear behavior of light-cured packable composite resins. *Dent Mater* 2000; 16: 33-40.
- 24) Fano L, Fano V, Ma W, Wang X, Zhu F. Hydrolytic degradation and cracks in Resin-modified glass-ionomer cements. *J Biomed Mater Res Part B: Appl Biomater* 2004; 87-93.

# Twenty-four Hour Flexural and Shear Bond Strengths of Flowable light-cured Composites : A Comparison Analysis Using Weibul Statistics

## ORIGINALITY REPORT

13%

SIMILARITY INDEX

5%

INTERNET SOURCES

10%

PUBLICATIONS

6%

STUDENT PAPERS

## PRIMARY SOURCES

- 1 Hyeongjik Lee, Jonghyun Shin, Jiyeon Kim, Taesung Jeong, Shin Kim. "Shear Bond Strength of a 3-in-1 Flowable Composite Resin to Primary Teeth", THE JOURNAL OF THE KOREAN ACADEMY OF PEDTATRIC DENTISTRY, 2018  
Publication 1%
- 2 McCabe, J.F.. "A statistical approach to the mechanical testing of dental materials", Dental Materials, 198608  
Publication 1%
- 3 Finger, W.J.. "Monomers with low oxygen inhibition as enamel/dentin adhesives", Dental Materials, 199607  
Publication 1%
- 4 Submitted to Mahidol University  
Student Paper 1%
- 5 M.J. Cattell, R.P. Palumbo, J.C. Knowles, R.L. 1%